


# **Imaging Solutions for Stem Cell Research**


**Cell Culture Observation System** 

BioStation CT

Cell Tracker



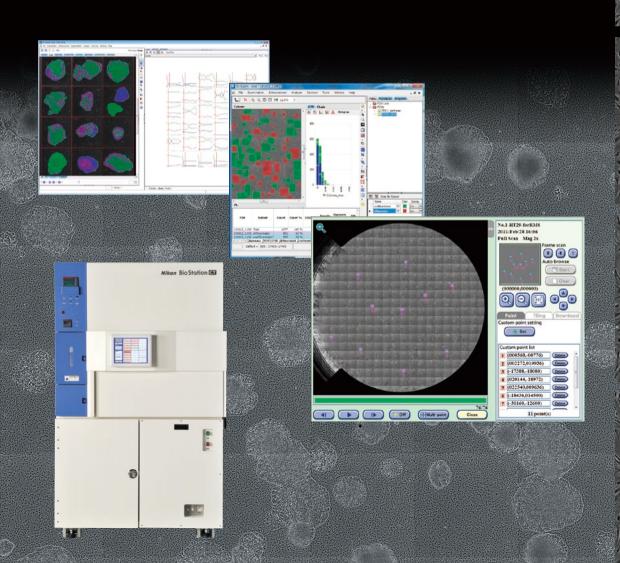

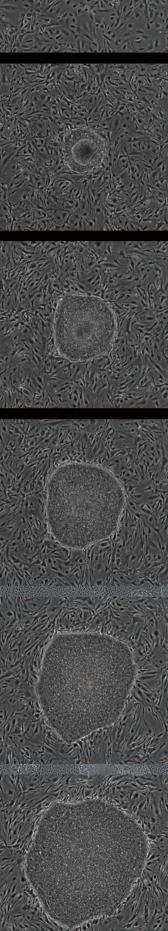

# **Stem cell screening inside the incubator**

With conventional cell monitoring procedures, a culture vessel has to be taken out of the incubator for microscope observation, where cells are subjected to stressful environmental changes and vibration. Researchers then have to spend additional time repositioning the vessel to find the same observation points. Nikon's BioStation CT eliminates these problems by providing a stable environment so that the cultures don't suffer while they are being imaged and allowing for a complete trace of the same live cells, including stem cells.

#### Advanced basic functions

#### **Automatic image capture**


The autofocus mechanism allows the capture of in-focus images. Z-stack imaging in phase contrast observation, multi-sample imaging and multi-point imaging are possible with multiple magnifications. User-configured imaging

conditions that can be saved in BioStation CT support the repeatability of observations.




#### Remote access

Configuring the imaging settings, scheduling a time-lapse experiment, and viewing the cell images are possible via a network. The captured data can be automatically downloaded to the user's local computer. This enables users to monitor the cell status away from the laboratory. When a culture environment (temperature, humidity, CO<sub>2</sub> concentration) control error occurs, BioStation CT can notify the users of the error by e-mails.

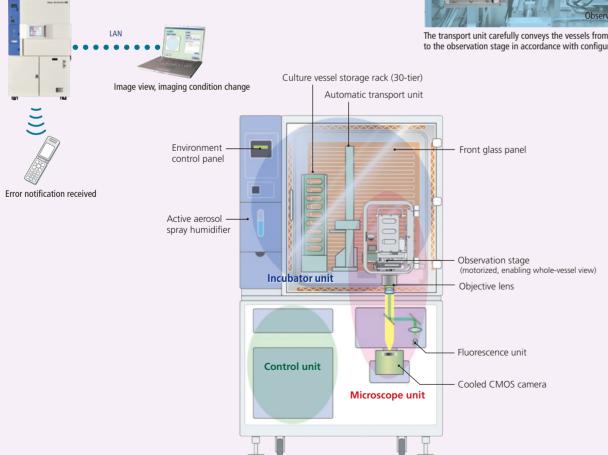

## **Automatic vessel transportation**

BioStation CT incorporates a transport unit that provides stable vessel transportation within the heated and humidified incubation area. The high-precision motorized stage in the observation unit allows for automated imaging of the entire area of a well in all culturing formats.





The transport unit carefully conveys the vessels from the storage rack to the observation stage in accordance with configured schedules.


#### Various functions

#### Full-well scan imaging and highly magnified image stitching

High-resolution full-well scans are reconstructed by stitching captured adjacent images. This enables clear detection of an iPS colony, which is difficult to detect because of its low induction efficiency, no matter where it forms in the vessel. The specified position of the vessel can be highly magnified with high resolution. BioStation CT also offers cell registration to allow for repeated visits to the same location. These time-lapse sequences can be created even when a vessel is removed from the BioStation CT for medium exchange.









Mouse iPS cells reprogramming GFP: Nanog-GFP DsRed: retrovirally transduced Vessel: 100 mm culture dish Magnification: 2x

Culture period: 3 weeks Imaging interval: 4 hours Courtesy of Dr. Hidemasa Kato, Saitama Medical

Day 5 of culture

Day 13 of culture

Day 18 of culture


#### Fluorescence observation

Long-life and low-cost LED illuminator is employed as a light source. Up to five fluorescence filter cubes can be mounted. Up to three channels can be used with simultaneous multi-channel acquisition. The expression of fluorescence proteins such as CFP, YFP, Kusabira Orange, DsRed, Texas Red and Cy5 can be observed effectively in fluorescence observation.



#### **High S/N ratio image acquisition**

Thanks to the built-in cooled CMOS camera, low-noise images with an S/N ratio two times higher than conventional cameras can be acquired.




iPS colony acquired with a built-in camera

#### **Reduced phototoxicity**

The excitation period is shortened by synchronizing the camera exposure with the excitation illuminator. This prevents photobleaching of the specimen and minimizes the phototoxic damage on the cells.


#### Micro observation

Phase contrast and fluorescence images can be captured with the high-sensitivity cooled CMOS camera. These images can be magnified in 2x, 4x, 10x, 20x and 40x. Up to 40 phase contrast images can be captured along the Z axis with the Z-stack function.

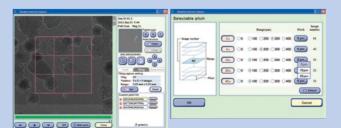

#### **Macro observation**

Brightfield image of the whole vessel provides users outside the BioStation CT with information such as handwritten information on the vessel, medium color and whether mold is growing or not. In addition, alkaline phosphatase stained cell counting is available as an option.





**Hypoxic culture capability** 

**Environment data recording** 

30min 2h - th

The culture environment is constantly monitored and recorded. The environment data can be accessed at

Hypoxic culture observation is possible with the optional oxygen regulator and nitrogen generator.

#### **Precise temperature control**

The inside temperature is directly controlled by panel heaters embedded in the incubator's six sides. This allows highly precise temperature maintenance.

#### Humidity control with air-flow type active aerosol spray humidifier

Distilled water is automatically sprayed inside the incubator to keep the optimum humidity. Water can be supplied to the tank without opening the incubator door. This air-flow type humidifier reduces contamination risks compared to the water bath type.

# 

12-well plate Up to 25 observation points in a well

100 mm culture dish



Up to 30 plates stored in a storage rack Up to 30 plates stored in a storage rack Up to 30 plates stored in a storage rack

48-well plate

**Compatible with various culture vessels** 

Up to 25 observation points in a well



24-well plate

Up to 25 observation points in a well

Up to 30 dishes stored in a storage rack 
Up to 60 dishes stored in a storage rack 
Up to 150 dishes stored in a storage rack Up to 25 observation points in a dish Up to 25 observation points in a dish Up to 25 observation points in a dish



25 cm<sup>2</sup> culture flask Up to 30 flasks stored in a storage rack

Up to 30 flasks stored in a storage rack 

#### Tray holders for various culture vessel types



For 100 mm culture dish



For well plate For 60 mm culture dishes





For nunc 60 mm culture dishes For 35 mm culture dishes



For 75 cm<sup>2</sup> culture flask

For 25 cm<sup>2</sup> culture flask

60 mm culture dish



#### Different GUI for each vessel type



Vessel type icons



GUI for 12-well plate

touchscreen.

# Easy operations

Close @ @

CO2 incubator environmental graph screen

Culture vessel installation into the

Vessels are placed in the incubator through a small door in

the front glass panel, minimizing negative effects on the

incubator

environment within the incubator.


#### **Vessel installation**

#### **Imaging parameter setting**

Smooth vessel transportation

than 2 mm. The drift and stress of cells are reduced.

The waver of liquid surface during the transportation is less



Fluorescence channel

#### Easy touchscreen operation

Time-lapse imaging configurations such as magnification, imaging point, fluorescence channel and stage motion speed can

# 15 min / Rose Small 1 Holder(t) (E) N (I) Toroleon Rounds 50 Set Section 40 15th 15th

Scheduling

#### Time-lapse imaging schedule


duced contamination risk The incubator interior can be sterilized using

rogen peroxide gas. (This is optional, and a

200 V power source is necessary.)

The imaging interval and total period can be set. The shortest time-lapse imaging interval is one minute.

**Captured image view** 



Macro image thumbnail

The time-course change of a specimen can be observed easily in sequentially displayed captured images.

#### **Medium exchange**

**High-precision repeatability** 

well as X-Y positions for each vessel.

Accurate tracing of same cells, even after medium exchange, is

possible using a dedicated tray holder, as BioStation CT records

culture history, such as medium exchange and subculture, as

Go to


1 Delete

#### **Data report**

#### Reliable data management and documentation support

Obtained data is duplicated and protected using uninterruptible power supply. Observation information such as temperature, humidity and imaging date can be written and displayed on the captured image to simplify presentation document preparation.

#### Imaging date and time Sample name




Imaging point within the vessel

#### **Culture history data management**

#### iPSC/non-iPSC Auto Identification

**CL Quant** 

Nikon co-developed an optional program for the BioStation CT with Kyoto University that automatically identifies colonies of iPS cells and counts them based on the structure of each colony. This method acquires data faster and increases its reliability. The iPS/non-iPS cell colony auto identification program saves times when evaluating large quantities of samples.

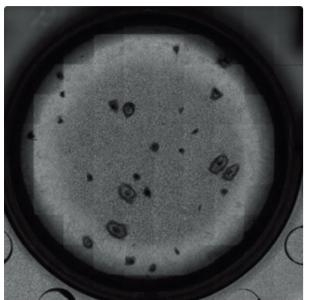



iPS cells

Image captured by the BioStation CT (magnification: 2×)

Image of iPS cells automatically distinguished from other cells using the iPS/non-iPS cell colony auto identification program

Showing the correlation between visual counts (vertical axis) and BioStation CT count (horizontal axis).

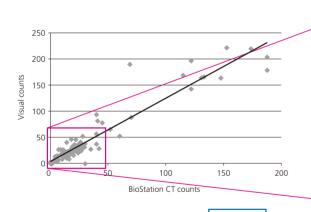

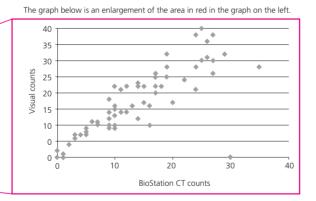



Counting colonies using the BioStation CT Source: Tatsuya Yamakawa, CiRA, Kyoto University  $R^2 = 0.904$  The correlation coefficient of 0.904 is high.

#### **Alkaline Phosphatase (AP)-positive Colony Counting**

**CL Quant** 


BioStation CT offers alkaline phosphatase-positive colony counting in macro images captured after AP staining, which enables valuation of the undifferentiated stem cell state.






AP-positive colony area comparison in 12 100 mm culture dishes Courtesy of Dr. Kazutoshi Takahashi and Mr. Koji Tanabe, Department of Reprogramming Science, Center for iPS Cell Research and Application (CiRA), Kyoto University

#### Reprogramming






Murine embryonic fibroblasts expressing transgenic oct4sox2-klf4-iresCherry and carrying an oct4-egfp reporter Full well scan at 2X and magnified view of reprogrammed colonies in phase, GFP, and DsRed Courtesy of Dr. Konrad Hochedlinger, Professor of Medicine, Harvard Medical School

### **iPS Colony Tracking Analysis**

**CL Quant** 

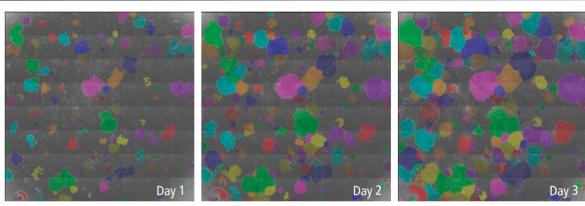

These whole images of 201B7 cell colonies grown in a 6-well-plate coated with fibronectin in the presence of drugs in hESF9 medium were measured by analysis software CLQuant. This assay can detect each iPS colony by recognizing the boundary even when confluent.


Magnification: 4x


Culture period: four days


Imaging interval: 12 hours


Courtesy of Dr. Miho K Furue (Project Leader) and Mr. Masaki Kinehara (2010-2013), National Institute of Biomedical Innovation (Japan)

#### **Apoptosis**









The apoptosis process of human ES cell line H9 cultured in the presence of MEF-CM on Matrigel® was observed. Annexin V (red fluorescence) was used as a detection probe for the cell membrane change that was caused by added BMP4.


Courtesy of Mr. Jamie McNicol, McMaster University

6


#### **Neural Stem Cells Direct Differentiation**

**Fibroblast** 

#### Neurosphere formation (neural stem cells)



**Neurite elongation** 



Imaging of the direct induction from mouse fibroblasts to neural stem cells and neurons


Magnification: 4x Culture period: 18 days Imaging interval: 4 hours

Stem Cells. 2012 Jun;30(6):1109-19

Courtesy of Prof. Hideyuki Okano and Dr. Takeshi Matsui Department of Physiology, Keio University School of Medicine

Day 9

#### **Dendrite Detection CL Quant**





The neurons are generated by directed differentiation of human iPS cells to neurons. A plasmid containing GFP (under EF1 promoter) was transfected. The dendrite length was measured with the image analysis software CL-Quant. The software can detect the dendrite (green), cell body (purple) and branch points (red).


Day 18

Magnification: 10x (fluorescence) Culture period: 19 hours Imaging interval: 10 min

Courtesy of Prof. James Ellis (Hospital for Sick Children-Toronto) and CCRM








Cell body

**Projection points** 


#### **Direct Induction (Chondrocytes)**

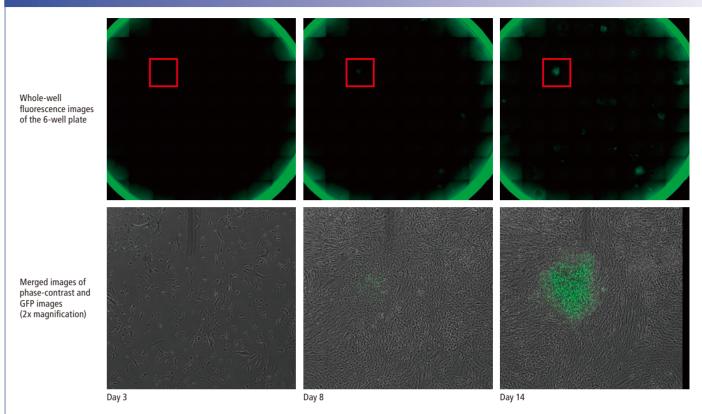


The time-lapse imaging of direct induction of chondrogenic cells from Human Dermal Fibroblast (HDF) cultured by defined factors. The forced expression of two reprogramming factors (c-Myc and Klf4) and one chondrogenic factor (SOX9) can induce chondrogenic (iChon) cells from HDF culture without going through a pluripotent state. The human iChon cells expressed marker genes for chondrocytes (COL11A2-GFP).

Courtesy of Professor Noriyuki Tsumaki, Department of Cell Growth and Differentiation, Center for iPS Cell Research and Application (CiRA), Kyoto University PLoS ONE 8(10): e77365.

#### **Differentiation Induction (Skeletal muscle)**

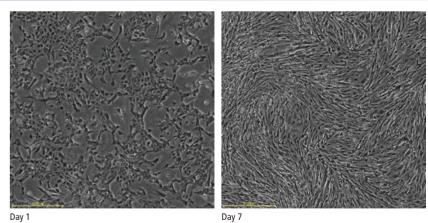

Human iPSCs (MyoD-hiPSs) changed their shape uniformly to spindle-like during differentiation from Day 1 to Day 7.



Functional assay for differentiated MyoD-hiPSCs. Serial photographs of differentiated MyoD-hiPSCs co-cultured with C2C12 cells (mouse myoblast cell line). A hiPSC-derived mCherry+ cell (red arrow) fused with a mousederived GFP+ cell (white arrow), resulting in a yellow cell (yellow arrow). This phenomenon is a characteristic of skeletal myocytes.


Courtesy of Dr. Hidetoshi Sakurai, Department of Clinical Application, Center for iPS Cell Research and Application (CiRA), Kyoto University PLoS ONE 8(4): e61540

Dendrite


Differentiation research Cancer and other research areas

#### **Hematopoietic Colony Forming Cell Assay**





(A) End-point colony identification and enumeration using the CL-Quant algorithm was compared to manual colony scoring (n=10). (B) The CL Quant algorithm produced a strong correlation to the total colony numbers quantified by manual counts (R2 = 0.917). (C, D, E) Correlations are shown between the algorithm-generated counts and the manual counts for each of the three major colony types: (C) CFU-E/BFU-E; (D) CFU-G/CFU-M; (E) CFU-GEMM.






Red/dark colonies (CFU-E/ BFU-E) Colony forming unit-erythroid (CFU-E) Burst forming unit-erythroid (BFU-E)





White colonies (CFU-M/ CFU-G) Colony forming unit-macrophage (CFU-M) Colony forming unit-granulocyte (CFU-G)



Mixed colonies containing both types on left (CFU-GEMM) Colony forming unit-granulocyte/erythroid/ macrophage/ megakaryocyte (CFU-GEMM)








#### **Mobility Analysis**


#### **CL Quant**

The distance of RCC4 cells (human renal cell carcinoma) was quantified by tracking (red line) the positions of cell centroids (green circle) using CL-Quant software. This assay could quantify the effect of adding Rapamycin or PP24.

J Urol. 2013 May;189(5):1921-9.

Courtesy of Dr. Shintaro Maru, Department of Renal and Genitourinary surgery, Hokkaido






# Breast cancer cells (MDA-MB-231) migrating in a 3D matrigel. The cells stably express H2B-GFP which nicely shows the chromatin structures in the nuclei. Some cells divide into three daughter cells (white arrowhead) instead of two. Cell tracking, lineage analysis and directional analysis are possible when using image analysis software CL-Quant. Courtesy of Ivar Noordstra, Department of Cell Biology, Utrecht University (Netherlands) Directional Analysis Directional Analysis

#### **Scratch Assay**

#### **CL Quant**

The acellular areas are extracted from captured images, and the time course is quantified. This enables comparative analysis of cells' metastatic ability.





Inhibition of cell migration by the anti-cancer drug sunitinib (Sutent®) added to clear cell renal carcinoma cell line (KMRC-1) was quantified by scratch assay. Cellular areas in the images captured in three-hour-interval time-lapse observation by BioStation CT were quantified by image analysis software CL-Quant. Courtesy of Dr. Naohisa Tomosugi and Dr. Shintaro Maru, Division of Nephrology, Kanazawa Medical University

#### NIS-Elements and the BioStation CT





In addition to CL-Quant, all images acquired with BioStation CT can be analyzed using the Nikon software NIS-Elements in conjunction with the module HC/JOBS, giving high flexibility in analysis.

10 11


#### Specifications

Specifications	
Operation	With touchscreen LCD Controllable via a network-linked PC (with Internet Explorer® web browser)
Incubator volume	460 L
Temperature control	Direct control via heater panels 37 °C, controlled directly via heater panels
Humidity controll	Via aerosol spray humidifier Range: 70% to 95%, 1% increments
CO <sub>2</sub> concentration control	CO <sub>2</sub> supply: by external CO <sub>2</sub> gas cylinder connection Range: 0% to 20%, 0.1% increments
O <sub>2</sub> concentration control (optional)	Via optional nitrogen gas generator Range: 0% to 20%, 1% increments
Compatible culture vessels	Culture dish: ø35 mm, ø60 mm, ø100 mm Well plate: 6-well, 12-well, 24-well, 48-well, 96-well Culture flask: 25 cm², 75 cm²
Specimen storage rack	3 rows x 10 tiers (autoclave sterilizable)
Macro observation	Image capture of whole vessel with dedicated camera (bird's-eye view) Camera head: color CCD camera (1280 x 960 pixels) Brightfield: backlight illumination


Micro observation	Magnification: 2x, 4x, 10x, 20x, 40x Intermediate magnification: 0.5x, 1x, 2x, 4x Objective: 4x (Plan Apo DLL), 10x (Plan Fluor ADL) Camera head: cooled CMOS camera (1M pixels) Phase contrast: high-intensity red LED illumination, automatic phase ring changeover Epi-fluorescence: LED 438 nm, 472 nm, white light illumination (up to 5 fluorescence filter cubes mountable)
Observation range	X-Y: 120 x 90 mm Z: 4 mm
Z-axis focusing	Z-focus point is automatically detected by image contrast detection through Z-axis scanning
Observation	With touchscreen LCD or via network-linked PC
Power source	Voltage: 115, 230 VAC ± 10% Power consumption: 1300 VA (max.)
Weight	Approx. 470 kg
Operating environment	Temperature: 15 °C to 28 °C Humidity: max. 60% relative humidity (noncondensing)

- BioStation CT does not have special components to protect the operator from infection.
- To decontaminate inside of incubator, use dry type hydrogen peroxide gas decontaminator.

#### **Dimensional diagram**

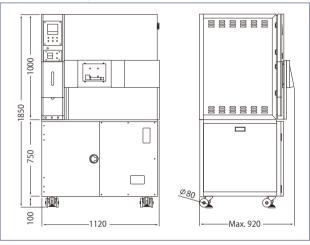

#### Hypoxic culture units dimensional diagrams

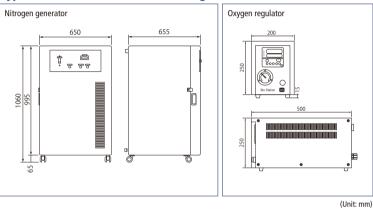

Cover image: courtesy of Dr. Ronald McKay, NIH

Specifications and equipment are subject to change without any notice or obligation on the part of the manufacturer. September 2015 @2007-15 NIKON CORPORATION



#### WARNING

TO ENSURE CORRECT USAGE, READ THE CORRESPONDING MANUALS CAREFULLY BEFORE USING YOUR EQUIPMENT.

Depending on the vessel used, the BioStation CT may not be able to focus on some areas External PC for data download is not included.

External PC for data download is not included. Repair of the machine under definite conditions is guaranteed by Nikon, but Nikon is not responsible for specimen and reagents. Monitor images are simulated. Company names and product names appearing in this brochure are their registered trademarks or trademarks. N.B. Export of the products 'in this brochure is controlled under the Japanese Foreign Exchange and Foreign Trade Law. Appropriate export procedure shall be required in case of export from Japan. 'Froducts: Hardware and its technical information (including software)



#### NIKON CORPORATION

Shinagawa Intercity Tower C, 2-15-3, Konan, Minato-ku, Tokyo 108-6290, Japan phone: +81-3-6433-3705 fax: +81-3-6433-3785 http://www.nikon.com/instruments/







ISO 14001 Certified for NIKON CORPORATION

#### NIKON INSTRUMENTS INC.

1300 Walt Whitman Road, Melville, N.Y. 11747-3064, U.S.A. phone: +1-631-547-8500; +1-800-52-NIKON (within the U.S.A. only) fax: +1-631-547-0306

http://www.nikoninstruments.com/

#### NIKON INSTRUMENTS EUROPE B.V.

Tripolis 100, Burgerweeshuispad 101, 1076 ER Amsterdam, The Netherlands phone: +31-20-7099-000 fax: +31-20-7099-298 http://www.nikoninstruments.eu/

#### NIKON INSTRUMENTS (SHANGHAI) CO., LTD.

CHINA phone: +86-21-6841-2050 fax: +86-21-6841-2060 (Beijing branch) phone: +86-10-5831-2028 fax: +86-10-5831-2026 (Guangzhou branch) phone: +86-20-3882-0550 fax: +86-20-3882-0580

#### NIKON SINGAPORE PTE LTD

SINGAPORE phone: +65-6559-3651 fax: +65-6559-3668

NIKON INSTRUMENTS KOREA CO., LTD. KOREA phone: +82-2-2186-8400 fax: +82-2-555-4415

#### NIKON CANADA INC.

CANADA phone: +1-905-602-9676 fax: +1-905-602-9953

#### NIKON FRANCE S.A.S.

FRANCE phone: +33-1-4516-45-16 fax: +33-1-4516-45-55

#### NIKON GMBH

GERMANY phone: +49-211-941-42-20 fax: +49-211-941-43-22

#### NIKON INSTRUMENTS S.p.A.

ITALY phone: +39-55-300-96-01 fax: +39-55-30-09-93

#### **NIKON AG**

SWITZERLAND phone: +41-43-277-28-67 fax: +41-43-277-28-61

#### NIKON UK LTD.

UNITED KINGDOM phone: +44-208-247-1717 fax: +44-208-541-4584

#### NIKON GMBH AUSTRIA

AUSTRIA phone: +43-1-972-6111-00 fax: +43-1-972-6111-40

#### NIKON BELUX

BELGIUM phone: +32-2-705-56-65 fax: +32-2-726-66-45

